Deep imaging with 1.3 μm dual-axis optical coherence tomography and an enhanced depth of focus: supplement

EVAN T. JELLY,[1,*] YANG ZHAO,[1] KENGYEH K. CHU,[1] HILLEL PRICE,[1] MICHAEL CROSE,[2] ZACHARY A. STEELMAN,[1] AND ADAM WAX[1]

[1]*Department of Biomedical Engineering, Duke University, Durham, NC 27708, USA*
[2]*Lumedica, Durham, NC 27701, USA*
*evan.jelly@duke.edu

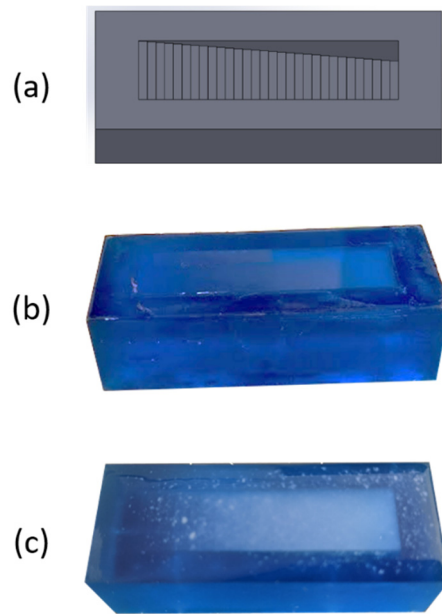# 1.3-μm dual-axis optical coherence tomography: supplemental document

Supplemental Figure S1

Fig. S1 (a) A 3d model of a step mold featuring cascading 250 ± 25 μm steps in the axial dimension ranging from 0-6 mm deep designed DA-OCT image depth performance characterization. (b) 3d-printed step resin mold filled with a Intralipid -based hydrogel optical scattering solution. (c) 3d-printed step resin mold filled with a hydrogel forward-scattering solution made featuring 25 μm polystyrene microspheres.